


Amendment to Page 44 – Imrie 3000

The **Briggs & Stratton** test diagram provided in the manual for the Imrie 3000 on page 44 is inaccurate. Below is the correct way to test this particular device:

Please note, this is Page 48 in the PDF Downloadable Manual.

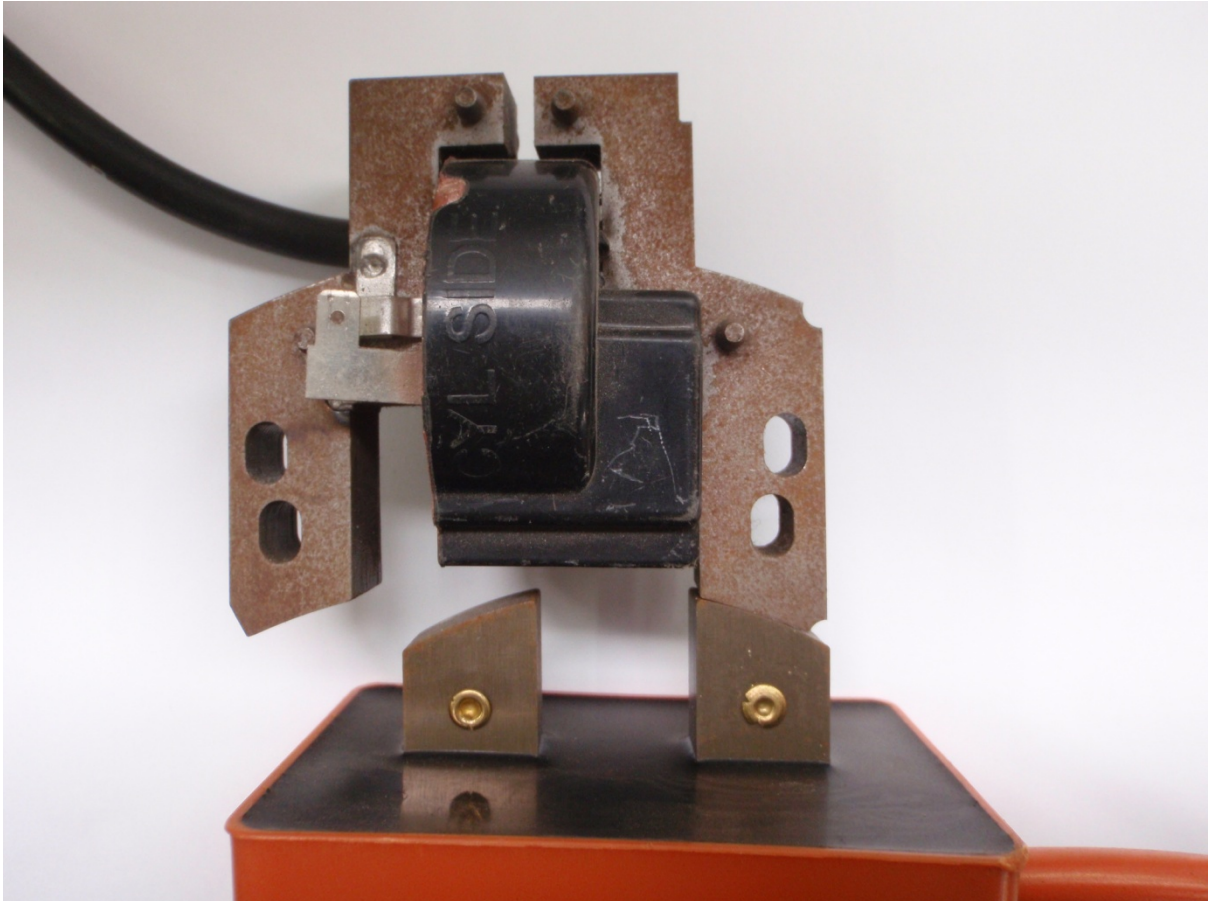

Imrie Diagnostic Testing apologises for any inconvenience this may have caused.